

Calibration Date: 9/8/2020

**Certificate of Calibration
of Volume Transfer**

Certificate Number: 2020-093-1

Items Submitted:

Quantity	Nominal Volume	Manufacturer	Type
2	100 gal	Seraphin / Detterman	Bottom Drain Prover

Submitted By: FSCP Area 70

3721 West Cuming St.
Lincoln, NE 68524

POC: Scott Arner

402-471-3422

scott.arner@nebraska.gov

Test Results

Nominal Volume	Serial Number	Material	Cubical Coefficient of Expansion (°F)	As Found Volume Delivered @ 60 °F	As left Volume Delivered @ 60 °F	Uncertainty (U)	(k)
100 gal	18969-S	304 SS	0.0000288	99.989 gal	99.989 gal	0.011 gal	2.01
100 gal	8851397-D	SS	0.0000265	100.012 gal	100.012 gal	0.011 gal	2.01

The data in this report only applies to those items specifically listed on this report.

Volume delivered at 60°F after a 30 second pour and 10 second drain for test measures. For provers a 30 second drain time would apply.

Conversion Factors:

1 gal = 231 in³

1 gal = 3.785 412 E-03 m³

Traceability Statement:

The artifact(s) described in this report have been compared to the Standards of the State of Nebraska. The Standards of the State of Nebraska are traceable to the International System of Units (SI) through the National Institute of Standards and Technology (NIST) and are part of a comprehensive measurement assurance program for ensuring continued accuracy and measurement traceability within the level of uncertainty reported by this laboratory. The calibration number for this report is the only unique calibration number to be used in referencing measurement traceability for the artifact(s) described in this report.

Uncertainty Statement:

The combined standard uncertainty includes uncertainties reported for the standard, uncertainties associated with the measurement process, uncertainties for any observed deviations from reference values which are less than surveillance limits and the standard uncertainty for any uncorrected errors. The combined standard uncertainty is multiplied by a coverage factor (k), to give the expanded uncertainty, which defines an interval with a 95.45 percent level of confidence. The expanded uncertainty presented in this report is consistent with the Guide to the Expression of Uncertainty in Measurement (2008, revised 2012). Some components of the calibration can be evaluated through a Type A evaluation, or the method of evaluation of uncertainty by the statistical analysis (standard deviation) from the observations taken.

Pertinent Information:

The artifact(s) listed above have been found and/or left within the maximum permissible error for the specification stated above, except as noted. An artifact is considered in-compliance when the correction plus the measurement uncertainty is equal to or less than the maximum permissible error. All of the tolerances and specifications were evaluated according to NIST HB 105-3 (2010).

Condition of Item(s) Submitted for Calibration:

Good

Laboratory Reference Standard Used:

100 gal NE 44158

Treatment of Item(s) before Calibration:

Tested as Found

Procedure Used:

NISTIR 7383, SOP 19 (2016)

Environmental conditions at time of calibration:


Temp °C	24.3	Humidity %	47.6
Pressure mmHg	731.01		

Water temperature at time of calibration:

68.67 °F

Date Submitted:

9/8/2020



Joel P. Lavicky, Metrologist

9/14/2020

Issue Date:

This document does not represent or imply endorsement by the State of Nebraska, the Nebraska Standards Laboratory or NIST. This document may not be reproduced, except in full, without the written permission of the Nebraska Standards Laboratory

Calibration Date: 9/14/2020

**Certificate of Calibration
of Volume Transfer**

Certificate Number: 2020-098-1

Items Submitted:

Quantity	Nominal Volume	Manufacturer	Type
1	500 gal	Unknown	Bottom Drain Prover

Submitted By: FSCP Area 70

3721 West Cuming St.
Lincoln, NE 68524

POC: Scott Arner
402-471-3422
scott.arner@nebraska.gov

Test Results

Nominal Volume	Serial Number	Material	Cubical Coefficient of Expansion (°F)	As Found Volume Delivered @ 60 °F	As left Volume Delivered @ 60 °F	Uncertainty (U)	(k)
500 gal	2024	MS	0.0000186	499.93 gal	499.93 gal	0.16 gal	2.02

The data in this report only applies to those items specifically listed on this report.

Volume delivered at 60°F after a 30 second pour and 10 second drain for test measures. For provers a 30 second drain time would apply.

Conversion Factors:

1 gal = 231 in³
1 gal = 3.785 412 E-3 m³

Traceability Statement:

The artifact(s) described in this report have been compared to the Standards of the State of Nebraska. The Standards of the State of Nebraska are traceable to the International System of Units (SI) through the National Institute of Standards and Technology (NIST) and are part of a comprehensive measurement assurance program for ensuring continued accuracy and measurement traceability within the level of uncertainty reported by this laboratory. The calibration number for this report is the only unique calibration number to be used in referencing measurement traceability for the artifact(s) described in this report.

Uncertainty Statement:

The combined standard uncertainty includes uncertainties reported for the standard, uncertainties associated with the measurement process, uncertainties for any observed deviations from reference values which are less than surveillance limits and the standard uncertainty for any uncorrected errors. The combined standard uncertainty is multiplied by a coverage factor (*k*), to give the expanded uncertainty, which defines an interval with a 95.45 percent level of confidence. The expanded uncertainty presented in this report is consistent with the Guide to the Expression of Uncertainty in Measurement (2008, revised 2012). Some components of the calibration can be evaluated through a Type A evaluation, or the method of evaluation of uncertainty by the statistical analysis (standard deviation) from the observations taken.

Pertinent Information:

The artifact(s) listed above have been found and/or left within the maximum permissible error for the specification stated above, except as noted. An artifact is considered in-compliance when the correction plus the measurement uncertainty is equal to or less than the maximum permissible error. All of the tolerances and specifications were evaluated according to NIST HB 105-3 (2010).

Condition of Item(s) Submitted for Calibration:

Good

Laboratory Reference Standard Used:

100 gal NE 44158

Treatment of Item(s) before Calibration:

Tested as Found

Procedure Used:

NISTIR 7383, SOP 19 (2016)


Environmental conditions at time of calibration:

Temp °C	23.2	Humidity %	40.6
Pressure mmHg	731.77		

Water temperature at time of calibration:

67.98 °F

Date Submitted: 9/14/2020



Joel P. Lavicky, Metrologist

9/14/2020

Issue Date:

This document does not represent or imply endorsement by the State of Nebraska, the Nebraska Standards Laboratory or NIST. This document may not be reproduced, except in full, without the written permission of the Nebraska Standards Laboratory

Calibration Certificate for Volume Transfer of LPG

Calibration Date: September 9, 2020

Certificate Number: 2020-093-2

Submitted by: FSCP Area 70
3721 West Cuming St.
Lincoln, NE 68524

POC: Scott Arner
Phone: 402-417-2087

Date Received: 09/08/2020

PO Number: N/A
Job Order #: N/A

Artifact(s) Description

Test Item(s): 103 gal LPG Prover
Serial No: A-4-L6998
Manufacture: Unknown
Condition: good

Material: Steel, Pressure Vessel, Low Carbon
Specification: NIST HB 105-4
Cubical Coefficient of Expansion: 0.000016 / °F

Calibration Information

Reference Standards Used:
NE-44158-100gal

Procedure: NIST SOP 21(2016)

NE-514-1 gal

Metrologist: JPL

Temperature: 19.7 °C

Humidity: 50.3 % RH

Water Temperature: 20.3 °C

Calibration Results

Nominal Volume (at zero mark on gauge)	Prover Volume As Found @ 60 °F and 100 psig (gal)	Prover Volume As Left @ 60 °F and 100 psig (gal)	Spec. Tol. ± (gal)	Uncertainty ± (gal)	k factor	Degrees of Freedom
103 gal	103.012	103.012	0.206	0.022	2	5716

Conversion Factors

1 gallon (U.S.) (gal) = 231 in³
1 gallon (U.S.) (gal) = 3.785 412 E-03 m³

Pertinent Information

- The artifact is considered in-tolerance when the error is equal to or less than the specified tolerance minus the measurement uncertainty. RED print indicates an out-of-tolerance reading. All of the tolerances and specifications were evaluated according to NIST HB 105-4 (2016)
- Enter the Pressure Correction from Table 1 that corresponds with the pressure being tested on your LPG Meter Test form.
- The calibration item was calibrated in a 'wet down' condition using water. The calibration data above applies when the prover bottom zero is obtained during a 30 (± 5) second period after cessation of the main flow.
- The drain time (using the on board pump) to the bottom zero was approximately 3 minute(s) 0 seconds.
- The Top Security Seal Number is "NE Lab" and the Bottom Security Seal Number is "NE Lab".

Traceability Statement

The artifact(s) described in this report have been compared to the Standards of the State of Nebraska. The Standards of the State of Nebraska are traceable to the SI through the National Institute of Standards and Technology (NIST) and are part of a comprehensive measurement assurance program for ensuring continued accuracy and measurement traceability within the level of uncertainty reported by this laboratory. The International System of Units (SI) for volume is the cubic meter (m³) (see Conversion Factors below). The report number for this report is the only unique report number to be used in referencing measurement traceability for the artifact(s) described in this report.

Uncertainty Statement

The combined standard uncertainty includes uncertainties for the standard(s), for the measurement process, for the material cubical coefficient of expansion, for reading meniscus, for the pressure gauge, for graduated neck errors and for the thermometer(s) used for measuring the water temperature. The combined standard uncertainty is multiplied by a coverage factor, *k*, to give the expanded uncertainty, which defines an interval with a 95.45 % level of confidence. The expanded uncertainty presented in this report is consistent with JCGM 100:2008, *Evaluation of measurement data — Guide to the expression of uncertainty in measurement (GUM 1995 with minor corrections)*. A component for the effects of viscosity was not included in the uncertainty budget.

Signature:

Date: 9/11/2020

Joel P. Lavicky, State Metrologist

The results in this certificate only applies to those items specifically listed in this certificate. The certificate cannot be considered complete unless it contains all pages. The document may not be reproduced except in full, without the written consent of the Nebraska Standards Laboratory

- Attachments: Table 1 and Chart 1 - LPG Prover Pressure Corrections
Table 2 - LPG Prover Temperature Corrections
Table 3 - Volume Corrections for Thermal Expansion or Contraction of Prover
Table 4 - Volume Correction Factors to 60 °F

LPG Prover Pressure Corrections

Attachment To Certificate No.: 2020-093-2

Calibration Date: September 9, 2020

Tested Item(s): 103 gal LPG Prover

Serial Number:

A-4-L6998

Table 1 - 103 gal LPG Prover Pressure Corrections @ 60 °F

psig	Prover Scale Reading (gal)	Pressure Correction (Pcorr) (gal)
20	0.135	-0.158
30	0.105	-0.132
40	0.075	-0.105
50	0.045	-0.078
60	0.026	-0.063
70	0.007	-0.047
80	-0.012	-0.031
90	-0.031	-0.016
100	-0.050	0.000
110	-0.070	0.017
120	-0.090	0.033
130	-0.110	0.050
140	-0.130	0.067
150	-0.150	0.083
160	-0.165	0.095
170	-0.180	0.107
180	-0.195	0.118
190	-0.210	0.130
200	-0.225	0.142

LPG Prover Pressure Corrections

Attachment To Certificate No.: 2020-093-2


Calibration Date: September 9, 2020

Tested Item(s): 103 gal LPG Prover

Serial Number:

A-4-L6998

Chart 1 - LPG Pressure Corrections (gal) @ 60 °F

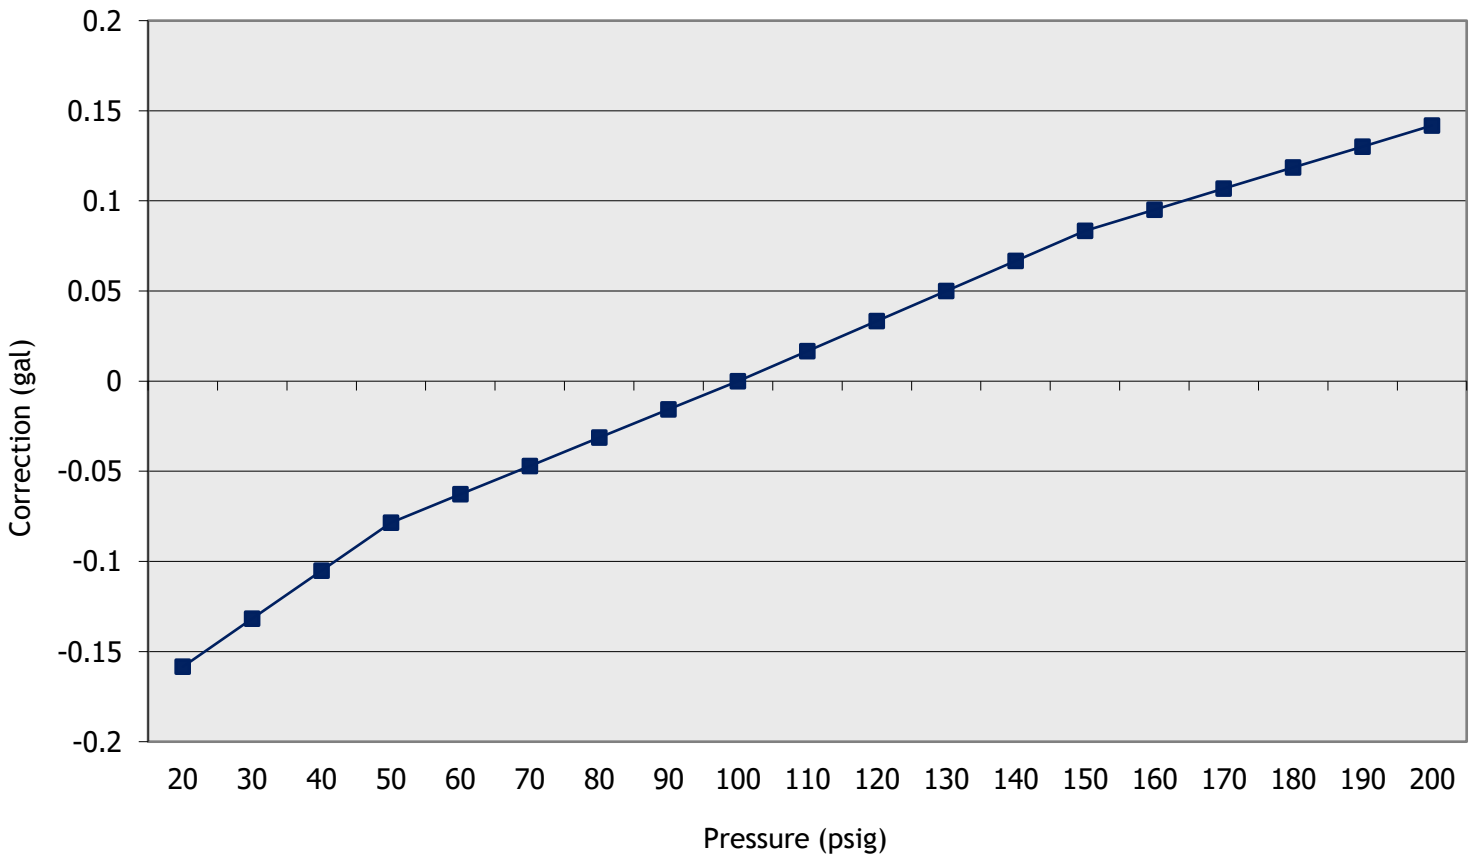

LPG Prover Temperature Corrections

Attachment To Certificate No.: 2020-093-2

Calibration Date: September 9, 2020

Tested Item(s): 103 gal LPG Prover

Serial Number: A-4-L6998

Table 2 - LPG Temperature Corrections

Correction Per °F Difference between Meter Temperature and Prover Temperature

Propane Specific Gravity 60/60 °F 0.505*

Liquid in Prover Temp. °F	in ³ / °F	gal / °F	Liquid in Prover Temp. °F	in ³ / °F	gal / °F	Liquid in Prover Temp. °F	in ³ / °F	gal / °F
0	35.578	0.1540	34	37.260	0.1613	68	39.305	0.1702
1	35.623	0.1542	35	37.314	0.1615	69	39.372	0.1704
2	35.669	0.1544	36	37.369	0.1618	70	39.440	0.1707
3	35.715	0.1546	37	37.424	0.1620	71	39.508	0.1710
4	35.761	0.1548	38	37.479	0.1622	72	39.577	0.1713
5	35.807	0.1550	39	37.535	0.1625	73	39.646	0.1716
6	35.854	0.1552	40	37.590	0.1627	74	39.716	0.1719
7	35.901	0.1554	41	37.646	0.1630	75	39.786	0.1722
8	35.947	0.1556	42	37.703	0.1632	76	39.856	0.1725
9	35.995	0.1558	43	37.760	0.1635	77	39.929	0.1729
10	36.043	0.1560	44	37.817	0.1637	78	40.001	0.1732
11	36.090	0.1562	45	37.875	0.1640	79	40.073	0.1735
12	36.138	0.1564	46	37.933	0.1642	80	40.146	0.1738
13	36.187	0.1567	47	37.991	0.1645	81	40.220	0.1741
14	36.235	0.1569	48	38.049	0.1647	82	40.294	0.1744
15	36.284	0.1571	49	38.108	0.1650	83	40.369	0.1748
16	36.333	0.1573	50	38.168	0.1652	84	40.444	0.1751
17	36.382	0.1575	51	38.228	0.1655	85	40.520	0.1754
18	36.431	0.1577	52	38.288	0.1657	86	40.596	0.1757
19	36.481	0.1579	53	38.348	0.1660	87	40.674	0.1761
20	36.531	0.1581	54	38.409	0.1663	88	40.752	0.1764
21	36.581	0.1584	55	38.470	0.1665	89	40.830	0.1768
22	36.632	0.1586	56	38.532	0.1668	90	40.909	0.1771
23	36.683	0.1588	57	38.594	0.1671	91	40.989	0.1774
24	36.734	0.1590	58	38.657	0.1673	92	41.069	0.1778
25	36.785	0.1592	59	38.719	0.1676	93	41.150	0.1781
26	36.837	0.1595	60	38.783	0.1679	94	41.232	0.1785
27	36.889	0.1597	61	38.846	0.1682	95	41.315	0.1789
28	36.941	0.1599	62	38.911	0.1684	96	41.398	0.1792
29	36.993	0.1601	63	38.975	0.1687	97	41.482	0.1796
30	37.046	0.1604	64	39.040	0.1690	98	41.567	0.1799
31	37.099	0.1606	65	39.106	0.1693	99	41.652	0.1803
32	37.152	0.1608	66	39.172	0.1696	100	41.739	0.1807
33	37.206	0.1611	67	39.238	0.1699			

* Approximate specific gravity for a commercial LPG product.

Volume Corrections for Thermal Expansion or Contraction of Prover

Attachment To Certificate No.: 2020-093-2

Calibration Date: September 9, 2020

Tested Item(s): 103 gal LPG Prover

Serial Number: A-4-L6998

Table 3 - Volume Corrections for Thermal Expansion or Contraction of Prover

Coefficient of Cubical Expansion = 0.000016 / °F

Temp. °F	Correction (in ³)	Correction (gal)	Temp. °F	Correction (in ³)	Correction (gal)	Temp. °F	Correction (in ³)	Correction (gal)
0	-22.8	-0.099	34	-9.9	-0.043	68	3.0	0.013
1	-22.5	-0.097	35	-9.5	-0.041	69	3.4	0.015
2	-22.1	-0.096	36	-9.1	-0.040	70	3.8	0.016
3	-21.7	-0.094	37	-8.8	-0.038	71	4.2	0.018
4	-21.3	-0.092	38	-8.4	-0.036	72	4.6	0.020
5	-20.9	-0.091	39	-8.0	-0.035	73	4.9	0.021
6	-20.6	-0.089	40	-7.6	-0.033	74	5.3	0.023
7	-20.2	-0.087	41	-7.2	-0.031	75	5.7	0.025
8	-19.8	-0.086	42	-6.9	-0.030	76	6.1	0.026
9	-19.4	-0.084	43	-6.5	-0.028	77	6.5	0.028
10	-19.0	-0.082	44	-6.1	-0.026	78	6.9	0.030
11	-18.7	-0.081	45	-5.7	-0.025	79	7.2	0.031
12	-18.3	-0.079	46	-5.3	-0.023	80	7.6	0.033
13	-17.9	-0.077	47	-4.9	-0.021	81	8.0	0.035
14	-17.5	-0.076	48	-4.6	-0.020	82	8.4	0.036
15	-17.1	-0.074	49	-4.2	-0.018	83	8.8	0.038
16	-16.8	-0.073	50	-3.8	-0.016	84	9.1	0.040
17	-16.4	-0.071	51	-3.4	-0.015	85	9.5	0.041
18	-16.0	-0.069	52	-3.0	-0.013	86	9.9	0.043
19	-15.6	-0.068	53	-2.7	-0.012	87	10.3	0.044
20	-15.2	-0.066	54	-2.3	-0.010	88	10.7	0.046
21	-14.8	-0.064	55	-1.9	-0.008	89	11.0	0.048
22	-14.5	-0.063	56	-1.5	-0.007	90	11.4	0.049
23	-14.1	-0.061	57	-1.1	-0.005	91	11.8	0.051
24	-13.7	-0.059	58	-0.8	-0.003	92	12.2	0.053
25	-13.3	-0.058	59	-0.4	-0.002	93	12.6	0.054
26	-12.9	-0.056	60	0.0	0.000	94	12.9	0.056
27	-12.6	-0.054	61	0.4	0.002	95	13.3	0.058
28	-12.2	-0.053	62	0.8	0.003	96	13.7	0.059
29	-11.8	-0.051	63	1.1	0.005	97	14.1	0.061
30	-11.4	-0.049	64	1.5	0.007	98	14.5	0.063
31	-11.0	-0.048	65	1.9	0.008	99	14.8	0.064
32	-10.7	-0.046	66	2.3	0.010	100	15.2	0.066
33	-10.3	-0.044	67	2.7	0.012			

Volume Correction Factors to 60 °F

Attachment To Certificate No.: 2020-093-2

Calibration Date: September 9, 2020

Tested Item(s): 103 gal LPG Prover **Serial Number:** A-4-L6998

Table 4 - Volume Correction Factors to 60 °F

Propane Specific Gravity 60/60 °F 0.505*

Temp. °F	Correction Factor	Temp. °F	Correction Factor	Temp. °F	Correction Factor	Temp. °F	Correction Factor
0	1.09008	26	1.05283	52	1.01293	78	0.96955
1	1.08869	27	1.05134	53	1.01133	79	0.96780
2	1.08729	28	1.04986	54	1.00973	80	0.96604
3	1.08590	29	1.04837	55	1.00812	81	0.96427
4	1.08449	30	1.04688	56	1.00651	82	0.96249
5	1.08309	31	1.04538	57	1.00489	83	0.96071
6	1.08168	32	1.04388	58	1.00326	84	0.95892
7	1.08027	33	1.04237	59	1.00163	85	0.95712
8	1.07889	34	1.04086	60	1.00000	86	0.95532
9	1.07744	35	1.03935	61	0.99836	87	0.95351
10	1.07602	36	1.03783	62	0.99671	88	0.95168
11	1.07460	37	1.03631	63	0.99506	89	0.94986
12	1.07317	38	1.03478	64	0.99340	90	0.94802
13	1.07174	39	1.03325	65	0.99174	91	0.94617
14	1.07031	40	1.03172	66	0.99007	92	0.94432
15	1.06887	41	1.03018	67	0.98840	93	0.94246
16	1.06743	42	1.02863	68	0.98671	94	0.94059
17	1.06599	43	1.02708	69	0.98503	95	0.93871
18	1.06454	44	1.02553	70	0.98333	96	0.93682
19	1.06309	45	1.02397	71	0.98163	97	0.93493
20	1.06163	46	1.02241	72	0.97993	98	0.93302
21	1.06017	47	1.02084	73	0.97821	99	0.93110
22	1.05871	48	1.01927	74	0.97649	100	0.92918
23	1.05725	49	1.01769	75	0.97477		
24	1.05578	50	1.01611	76	0.97307		
25	1.05430	51	1.01452	77	0.97130		

* Approximate specific gravity for a commercial LPG product.

Calibration Certificate for Volume Transfer of LPG

Calibration Date: September 11, 2020

Certificate Number: 2020-093-3

Submitted by: FSCP Area 70
3721 West Cuming St.
Lincoln, NE 68524

POC: Scott Arner
Phone: 402-417-2087

Date Received: 09/08/2020

PO Number: N/A
Job Order #: N/A

Artifact(s) Description

Test Item(s): 20 gal LPG Prover
Serial No: 88220
Manufacture: Midwest Meter
Condition: good

Material: Steel, Pressure Vessel, Low Carbon
Specification: NIST HB 105-4
Cubical Coefficient of Expansion: 0.000016 / °F

Calibration Information

Reference Standards Used:

NE-1586-5 gal

Procedure: NIST SOP 21(2016)

Metrologist: JPL

Temperature: 19.7 °C

Humidity: 50.3 % RH

Water Temperature: 19.9 °C

Calibration Results

Nominal Volume (at zero mark on gauge)	Prover Volume As Found @ 60 °F and 100 psig (gal)	Prover Volume As Left @ 60 °F and 100 psig (gal)	Spec. Tol. ± (gal)	Uncertainty ± (gal)	k factor	Degrees of Freedom
20 gal	20.007	20.007	0.04	0.022	2.014	179

Conversion Factors

1 gallon (U.S.) (gal) = 231 in³
1 gallon (U.S.) (gal) = 3.785 412 E-03 m³

Pertinent Information

- The artifact is considered in-tolerance when the error is equal to or less than the specified tolerance minus the measurement uncertainty. **RED** print indicates an out-of-tolerance reading. All of the tolerances and specifications were evaluated according to NIST HB 105-4 (2016)
- Enter the Pressure Correction from Table 1 that corresponds with the pressure being tested on your LPG Meter Test form.
- The calibration item was calibrated in a 'wet down' condition using water. The calibration data above applies when the prover bottom zero is obtained during a 30 (± 5) second period after cessation of the main flow.
- The drain time (using gravity) to the bottom zero was approximately 2 minute(s) 30 seconds.
- The Top Security Seal Number is "NE Lab" and the Bottom Security Seal Number is "NE Lab".


Traceability Statement

The artifact(s) described in this report have been compared to the Standards of the State of Nebraska. The Standards of the State of Nebraska are traceable to the SI through the National Institute of Standards and Technology (NIST) and are part of a comprehensive measurement assurance program for ensuring continued accuracy and measurement traceability within the level of uncertainty reported by this laboratory. The International System of Units (SI) for volume is the cubic meter (m³) (see Conversion Factors below). The report number for this report is the only unique report number to be used in referencing measurement traceability for the artifact(s) described in this report.

Uncertainty Statement

The combined standard uncertainty includes uncertainties for the standard(s), for the measurement process, for the material cubical coefficient of expansion, for reading meniscus, for the pressure gauge, for graduated neck errors and for the thermometer(s) used for measuring the water temperature. The combined standard uncertainty is multiplied by a coverage factor, *k*, to give the expanded uncertainty, which defines an interval with a 95.45 % level of confidence. The expanded uncertainty presented in this report is consistent with JCGM 100:2008, *Evaluation of measurement data — Guide to the expression of uncertainty in measurement (GUM 1995 with minor corrections)*. A component for the effects of viscosity was not included in the uncertainty budget.

Signature:



Joel P. Lavicky, State Metrologist

Date:

9/11/2020

The results in this certificate only applies to those items specifically listed in this certificate. The certificate cannot be considered complete unless it contains all pages. The document may not be reproduced except in full, without the written consent of the Nebraska Standards Laboratory

- Attachments: Table 1 and Chart 1 - LPG Prover Pressure Corrections
Table 2 - LPG Prover Temperature Corrections
Table 3 - Volume Corrections for Thermal Expansion or Contraction of Prover
Table 4 - Volume Correction Factors to 60 °F

LPG Prover Pressure Corrections

Attachment To Certificate No.: 2020-093-3

Calibration Date: September 11, 2020

Tested Item(s): 20 gal LPG Prover

Serial Number:

88220

Table 1 - 20 gal LPG Prover Pressure Corrections @ 60 °F

psig	Prover Scale Reading (gal)	Pressure Correction (Pcorr) (gal)
20	0.020	-0.030
30	0.013	-0.024
40	0.007	-0.018
50	0.000	-0.012
60	-0.003	-0.009
70	-0.006	-0.007
80	-0.009	-0.005
90	-0.012	-0.002
100	-0.015	0.000
110	-0.017	0.001
120	-0.019	0.003
130	-0.021	0.004
140	-0.023	0.005
150	-0.025	0.007
160	-0.026	0.007
170	-0.027	0.007
180	-0.028	0.008
190	-0.029	0.008
200	-0.030	0.009

LPG Prover Pressure Corrections

Attachment To Certificate No.: 2020-093-3


Calibration Date: September 11, 2020

Tested Item(s): 20 gal LPG Prover

Serial Number:

88220

Chart 1 - LPG Pressure Corrections (gal) @ 60 °F

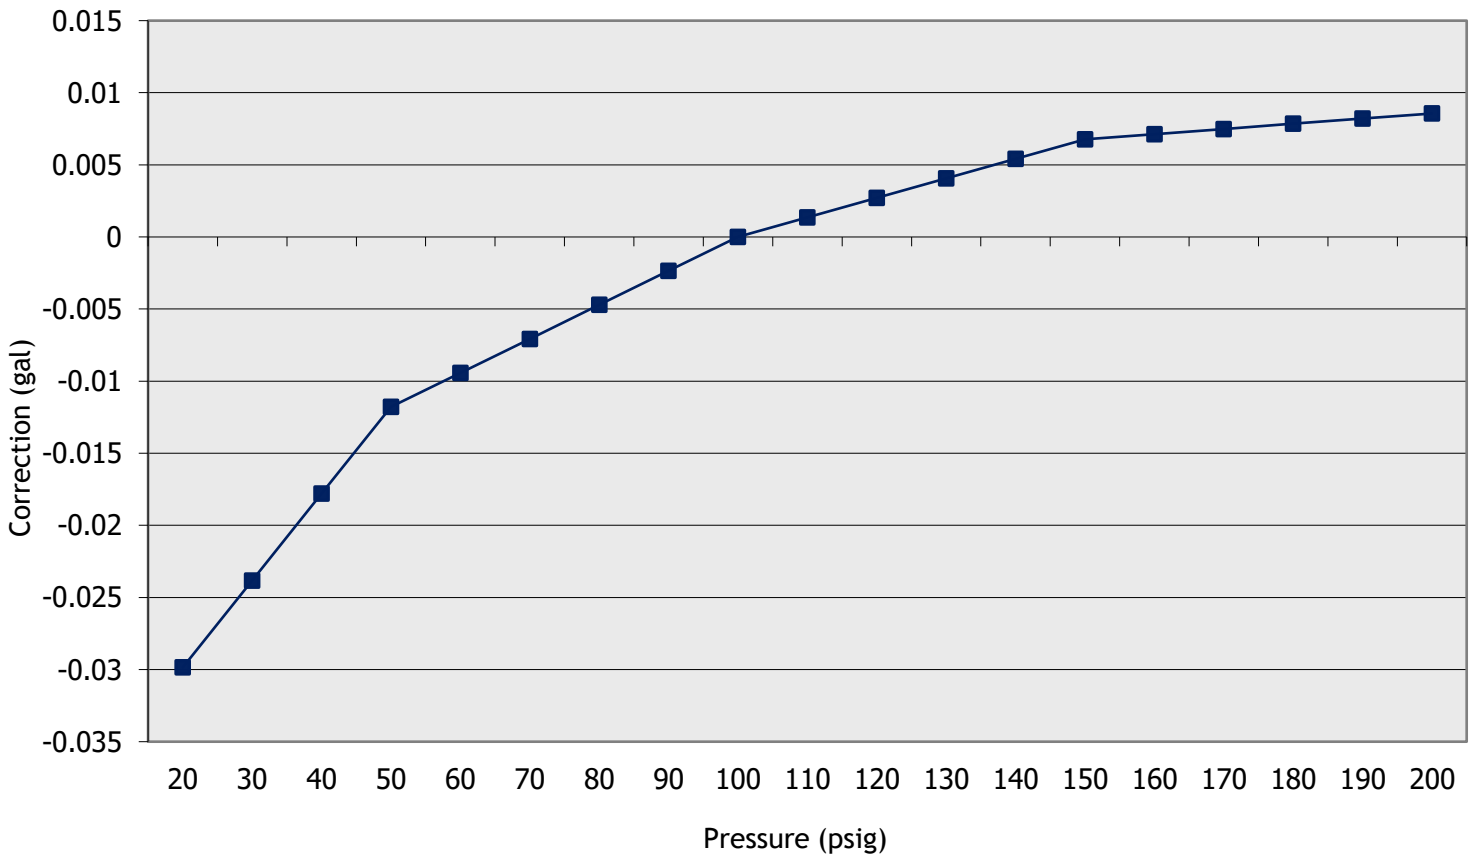



Good Life. Great Roots.

DEPARTMENT OF AGRICULTURE

Nebraska Standards Laboratory

3721 West Cuming St
Lincoln, NE 68524
(402)-471-2087

Director of Agriculture
Steve Wellman
P.O. Box 94947
Lincoln, NE 68509-4947
(402)-471-2341
www.nda.nebraska.gov

LPG Prover Temperature Corrections

Attachment To Certificate No.: 2020-093-3

Calibration Date: September 11, 2020

Tested Item(s): 20 gal LPG Prover

Serial Number: 88220

Table 2 - LPG Temperature Corrections

Correction Per °F Difference between Meter Temperature and Prover Temperature

Propane Specific Gravity 60/60 °F 0.505*

Liquid in Prover Temp. °F	in ³ / °F	gal / °F	Liquid in Prover Temp. °F	in ³ / °F	gal / °F	Liquid in Prover Temp. °F	in ³ / °F	gal / °F
0	6.908	0.0299	34	7.235	0.0313	68	7.632	0.0330
1	6.917	0.0299	35	7.245	0.0314	69	7.645	0.0331
2	6.926	0.0300	36	7.256	0.0314	70	7.658	0.0332
3	6.935	0.0300	37	7.267	0.0315	71	7.672	0.0332
4	6.944	0.0301	38	7.277	0.0315	72	7.685	0.0333
5	6.953	0.0301	39	7.288	0.0315	73	7.698	0.0333
6	6.962	0.0301	40	7.299	0.0316	74	7.712	0.0334
7	6.971	0.0302	41	7.310	0.0316	75	7.726	0.0334
8	6.980	0.0302	42	7.321	0.0317	76	7.739	0.0335
9	6.989	0.0303	43	7.332	0.0317	77	7.753	0.0336
10	6.999	0.0303	44	7.343	0.0318	78	7.767	0.0336
11	7.008	0.0303	45	7.354	0.0318	79	7.781	0.0337
12	7.017	0.0304	46	7.366	0.0319	80	7.795	0.0337
13	7.027	0.0304	47	7.377	0.0319	81	7.810	0.0338
14	7.036	0.0305	48	7.388	0.0320	82	7.824	0.0339
15	7.045	0.0305	49	7.400	0.0320	83	7.839	0.0339
16	7.055	0.0305	50	7.411	0.0321	84	7.853	0.0340
17	7.064	0.0306	51	7.423	0.0321	85	7.868	0.0341
18	7.074	0.0306	52	7.434	0.0322	86	7.883	0.0341
19	7.084	0.0307	53	7.446	0.0322	87	7.898	0.0342
20	7.093	0.0307	54	7.458	0.0323	88	7.913	0.0343
21	7.103	0.0307	55	7.470	0.0323	89	7.928	0.0343
22	7.113	0.0308	56	7.482	0.0324	90	7.944	0.0344
23	7.123	0.0308	57	7.494	0.0324	91	7.959	0.0345
24	7.133	0.0309	58	7.506	0.0325	92	7.975	0.0345
25	7.143	0.0309	59	7.518	0.0325	93	7.990	0.0346
26	7.153	0.0310	60	7.531	0.0326	94	8.006	0.0347
27	7.163	0.0310	61	7.543	0.0327	95	8.022	0.0347
28	7.173	0.0311	62	7.555	0.0327	96	8.038	0.0348
29	7.183	0.0311	63	7.568	0.0328	97	8.055	0.0349
30	7.193	0.0311	64	7.581	0.0328	98	8.071	0.0349
31	7.204	0.0312	65	7.593	0.0329	99	8.088	0.0350
32	7.214	0.0312	66	7.606	0.0329	100	8.105	0.0351
33	7.224	0.0313	67	7.619	0.0330			

* Approximate specific gravity for a commercial LPG product.

Volume Corrections for Thermal Expansion or Contraction of Prover

Attachment To Certificate No.: 2020-093-3

Calibration Date: September 11, 2020

Tested Item(s): 20 gal LPG Prover

Serial Number: 88220

Table 3 - Volume Corrections for Thermal Expansion or Contraction of Prover

Coefficient of Cubical Expansion = 0.000016 / °F

Temp. °F	Correction (in ³)	Correction (gal)	Temp. °F	Correction (in ³)	Correction (gal)	Temp. °F	Correction (in ³)	Correction (gal)
0	-4.4	-0.019	34	-1.9	-0.008	68	0.6	0.003
1	-4.4	-0.019	35	-1.8	-0.008	69	0.7	0.003
2	-4.3	-0.019	36	-1.8	-0.008	70	0.7	0.003
3	-4.2	-0.018	37	-1.7	-0.007	71	0.8	0.004
4	-4.1	-0.018	38	-1.6	-0.007	72	0.9	0.004
5	-4.1	-0.018	39	-1.6	-0.007	73	1.0	0.004
6	-4.0	-0.017	40	-1.5	-0.006	74	1.0	0.004
7	-3.9	-0.017	41	-1.4	-0.006	75	1.1	0.005
8	-3.8	-0.017	42	-1.3	-0.006	76	1.2	0.005
9	-3.8	-0.016	43	-1.3	-0.005	77	1.3	0.005
10	-3.7	-0.016	44	-1.2	-0.005	78	1.3	0.006
11	-3.6	-0.016	45	-1.1	-0.005	79	1.4	0.006
12	-3.5	-0.015	46	-1.0	-0.004	80	1.5	0.006
13	-3.5	-0.015	47	-1.0	-0.004	81	1.6	0.007
14	-3.4	-0.015	48	-0.9	-0.004	82	1.6	0.007
15	-3.3	-0.014	49	-0.8	-0.004	83	1.7	0.007
16	-3.3	-0.014	50	-0.7	-0.003	84	1.8	0.008
17	-3.2	-0.014	51	-0.7	-0.003	85	1.8	0.008
18	-3.1	-0.013	52	-0.6	-0.003	86	1.9	0.008
19	-3.0	-0.013	53	-0.5	-0.002	87	2.0	0.009
20	-3.0	-0.013	54	-0.4	-0.002	88	2.1	0.009
21	-2.9	-0.012	55	-0.4	-0.002	89	2.1	0.009
22	-2.8	-0.012	56	-0.3	-0.001	90	2.2	0.010
23	-2.7	-0.012	57	-0.2	-0.001	91	2.3	0.010
24	-2.7	-0.012	58	-0.1	-0.001	92	2.4	0.010
25	-2.6	-0.011	59	-0.1	0.000	93	2.4	0.011
26	-2.5	-0.011	60	0.0	0.000	94	2.5	0.011
27	-2.4	-0.011	61	0.1	0.000	95	2.6	0.011
28	-2.4	-0.010	62	0.1	0.001	96	2.7	0.012
29	-2.3	-0.010	63	0.2	0.001	97	2.7	0.012
30	-2.2	-0.010	64	0.3	0.001	98	2.8	0.012
31	-2.1	-0.009	65	0.4	0.002	99	2.9	0.012
32	-2.1	-0.009	66	0.4	0.002	100	3.0	0.013
33	-2.0	-0.009	67	0.5	0.002			

Volume Correction Factors to 60 °F

Attachment To Certificate No.: 2020-093-3

Calibration Date: September 11, 2020

Tested Item(s): 20 gal LPG Prover **Serial Number:** 88220

Table 4 - Volume Correction Factors to 60 °F

Propane Specific Gravity 60/60 °F 0.505*

Temp. °F	Correction Factor	Temp. °F	Correction Factor	Temp. °F	Correction Factor	Temp. °F	Correction Factor
0	1.09008	26	1.05283	52	1.01293	78	0.96955
1	1.08869	27	1.05134	53	1.01133	79	0.96780
2	1.08729	28	1.04986	54	1.00973	80	0.96604
3	1.08590	29	1.04837	55	1.00812	81	0.96427
4	1.08449	30	1.04688	56	1.00651	82	0.96249
5	1.08309	31	1.04538	57	1.00489	83	0.96071
6	1.08168	32	1.04388	58	1.00326	84	0.95892
7	1.08027	33	1.04237	59	1.00163	85	0.95712
8	1.07889	34	1.04086	60	1.00000	86	0.95532
9	1.07744	35	1.03935	61	0.99836	87	0.95351
10	1.07602	36	1.03783	62	0.99671	88	0.95168
11	1.07460	37	1.03631	63	0.99506	89	0.94986
12	1.07317	38	1.03478	64	0.99340	90	0.94802
13	1.07174	39	1.03325	65	0.99174	91	0.94617
14	1.07031	40	1.03172	66	0.99007	92	0.94432
15	1.06887	41	1.03018	67	0.98840	93	0.94246
16	1.06743	42	1.02863	68	0.98671	94	0.94059
17	1.06599	43	1.02708	69	0.98503	95	0.93871
18	1.06454	44	1.02553	70	0.98333	96	0.93682
19	1.06309	45	1.02397	71	0.98163	97	0.93493
20	1.06163	46	1.02241	72	0.97993	98	0.93302
21	1.06017	47	1.02084	73	0.97821	99	0.93110
22	1.05871	48	1.01927	74	0.97649	100	0.92918
23	1.05725	49	1.01769	75	0.97477		
24	1.05578	50	1.01611	76	0.97307		
25	1.05430	51	1.01452	77	0.97130		

* Approximate specific gravity for a commercial LPG product.